

Service Manual RD-4600

3 HP Automatic Control Under Counter Mount

Rev 5 - 1-14-20 900-097M

Installation

- Place the shipping carton in the desired location. Remove the unit from the shipping carton.
- 2. Remove the full sized mounting template from the service manual. Place in desired location and mark four places to be drilled. We recommend the faceplate to be offset inward 1/8" to no more then 1/4" from the front of the counters edge.
- 3. Pre-drill a hole 1/2" deep using a 5/32" drill bit. Do not drill through the counter top
- 4. Slide the unit apart by seperating the faceplate assembly from the fixed body assembly. With the unit fully extended, line up the outer chassis aligning the holes with the pre-drilled holes. Place a spacer in one corner to lightly fasten it using a phillips screw. Repeat the process until all four screws and spacers are installed. Tighten securly making sure the face plate slides in and out freely.
- 5. Insert the umbilical tubing in first and follow with the unit.



NOTE

This unit requires a regulated air and water supply. Filters are highly recommended.

- 6. Install optional master valve assemblies, with filter and regulator, onto the manual shut-off valves. (Pressures are preset at the factory: 80 psi air, 40 psi water).
- 7. Connect the supply tubings to the appropriate air and water supply lines.

Final <u>Adjustments</u>

Check air pressure, adjust to 80 psi if necessary. Check water pressure, adjust to 40 psi if necessary. Test handpieces for proper function. Test syringe for proper pressure and function.


- **Operation** 1. Turn on the master switch located on the right side of the faceplate.
 - The handpiece is automatically activated when lifted from the holder.
 - 3. Depress the foot control to activate each handpiece. Pressure is shown on the gauge for the handpiece being used.
 - 4. Individual handpiece pressure adjustments are located on the autoblock inside the unit. To adjust the pressure to each handpiece:
 - a. Turn adjustment screw *clockwise* to decrease the handpiece pressure.
 - b. Turn adjustment screw counter-clockwise to increase the handpiece pressure.

CAUTION

When adjusting the handpiece pressure, do not overtighten the screws. Damage may result.

- 5. Handpiece coolant water can be turned on or off with the toggle switch located in the lower center of the faceplate.
- 6. Water coolant flow adjustment is located to the right of the water coolant toggle switch.

Handpiece Purge The purge switch flushes fresh water through the water coolant system. Guidelines from the Center for Disease Control (CDC) recommends that each handpiece be flushed (purged) 20 to 30 seconds between patients and several minutes at the beginning of each day. Handpieces must be removed from the holder to activate the purge system.



Control Panel RD-4600

Troubleshooting

Symptom Handpiece lacks power.

Possible Causes

- A. Improper supply pressure from compressor (80 psi).
- B. Check handpiece pressure adjustment on unit.
- C. Air filter may be plugged.
- D. Pinched supply tubing.
- E. Defective handpiece gasket at connection with tubing.
- F. Defective handpiece.

Symptom

Water coolant does not shut off when foot control is released.

Possible Causes

- A. Adjust air pressure to 80 psi—water pressure to 40 psi.
- B. Foot control is not exhausting.
- Defective water relay valve.

Symptom

More than one handpiece is operating.

Possible Causes

- A. Handpiece is not all the way in the holder.
- B. Improper adjustment on pilot valve in the handpiece holder.
- C. Defective shuttle valve to gauge.

Symptom

Insufficient water coolant.

Possible Causes

- A. Adjust coolant flow valve.
- B. Water filter may be plugged.
- C. Handpiece may be plugged.
- D. Pinched supply tubing.
- E. Improper adjustment of water relay valve

Symptom

Water coolant is running from handpiece while in the holder.

Possible Causes


- A. Water pressure too high.
- B. Air pressure too low.
- C. Handpiece holder out of adjustment.


Symptom

Water coolant is running continuously.


Possible Causes

- A. Purge switch is on (on applicable systems).
- B. Water pressure to high.
- C. Handpiece holder out of adjustment.
- D. Defective water relay valve.

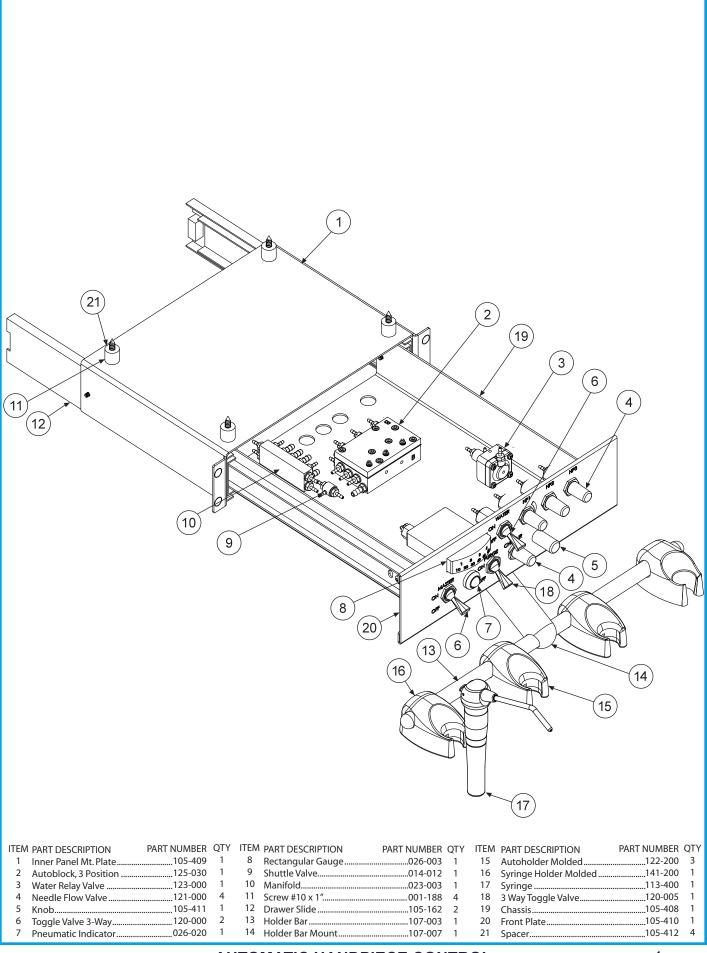


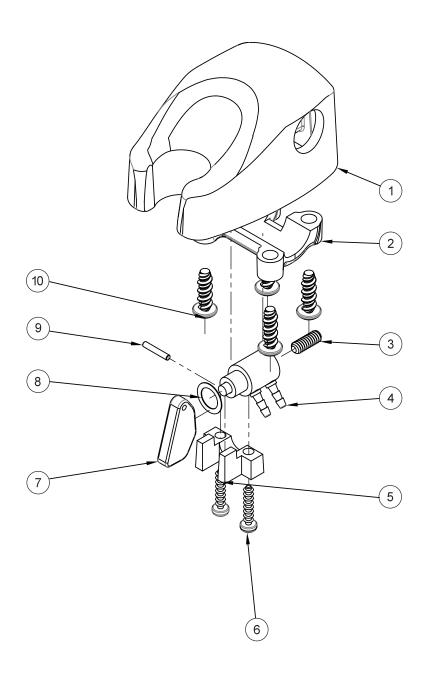



| ITEM | PART DESCRIPTION | PART NUMBER | QTY |
|------|-------------------------|-------------|-----|
| 1 | Molded Body | 122-201 | 1 |
| 2 | Clamp | 122-104 | 1 |
| 3 | Set Screw, 6-32 x 3/8" | 005-012 | 1 |
| 4 | Valve Cartridge | 122-031 | 1 |
| 5 | Molded Clip | 122-102 | 1 |
| 6 | Screw, 4 x 1/2" | 001-019 | 2 |
| 7 | Handpiece Actuator Leve | er122-103 | 1 |
| 8 | Washer | 003-004 | 1 |
| 9 | Pin, 1/16"x3/8" Dowel | 009-010 | 1 |
| 10 | Screw, 8-18 x 1/2" | 001-267 | 4 |
| | | | |

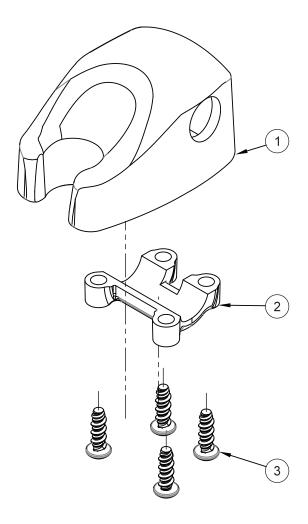



| ITEM | PART DESCRIPTION | PART NUMBER | QTY |
|------|--------------------|-------------|-----|
| 1 | Molded Body | 141-201 | 1 |
| 2 | Clamp | 122-204 | 1 |
| 3 | Screw, 8-32 x 1/2" | 001-267 | 4 |

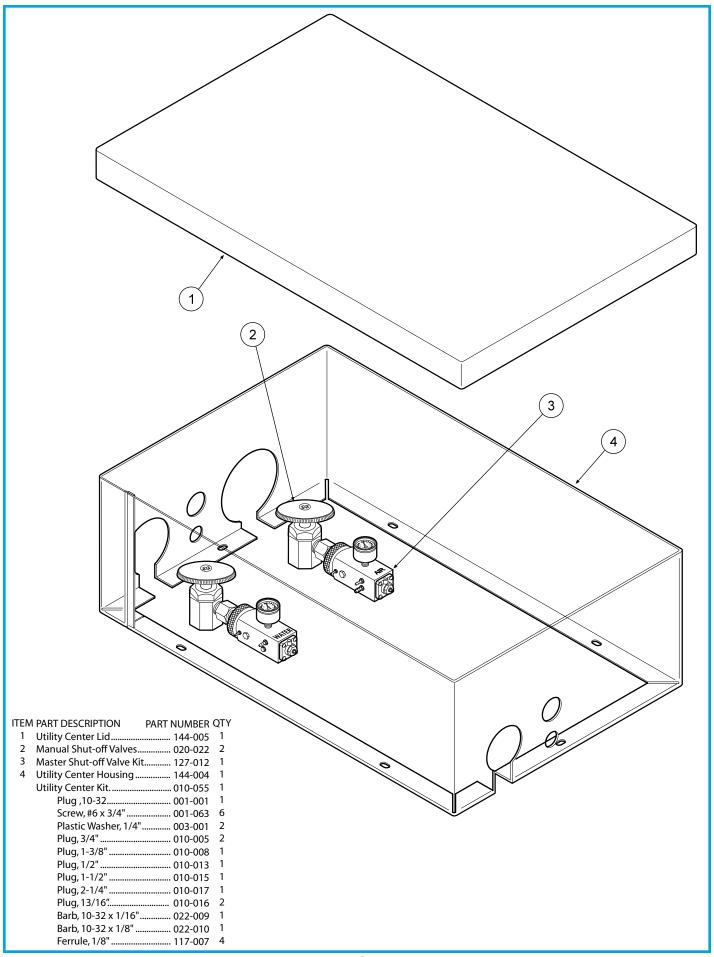


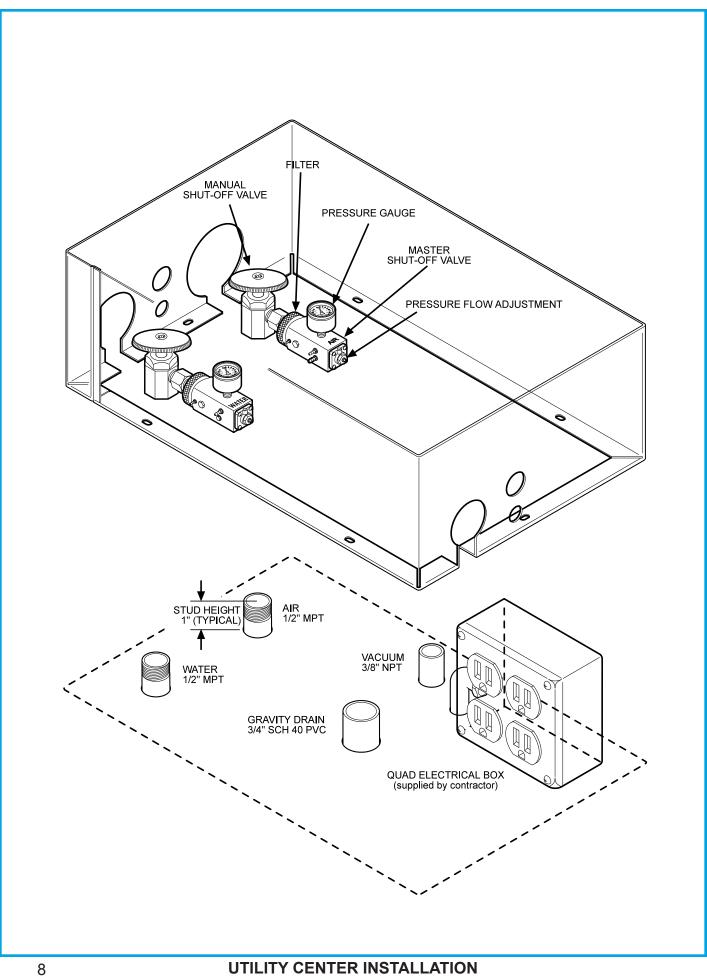

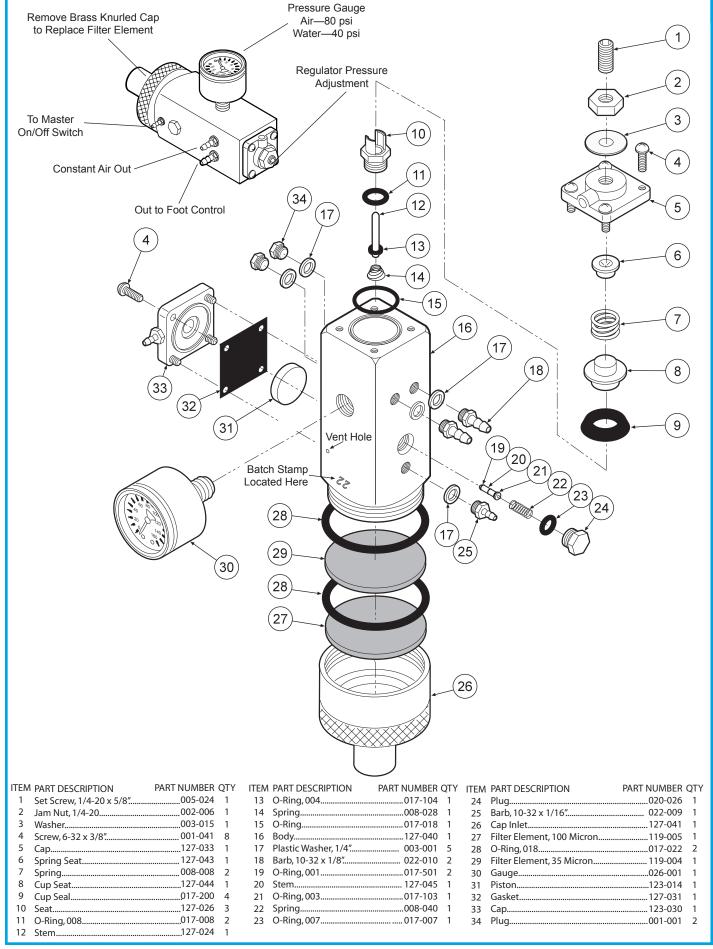

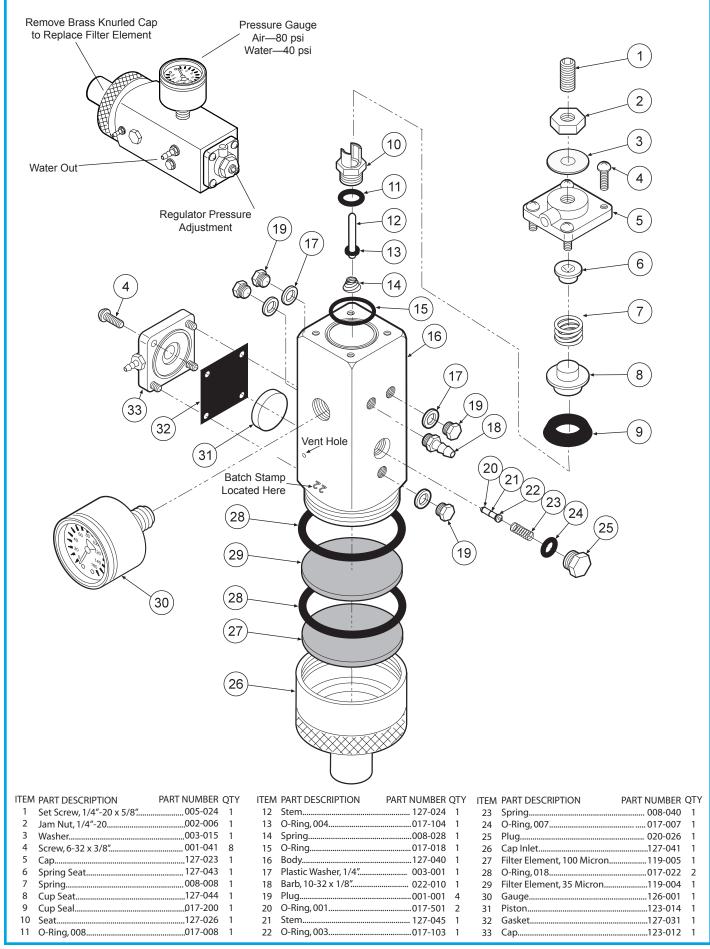


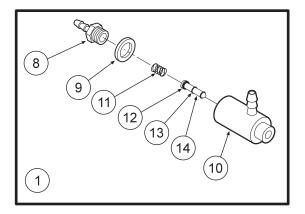


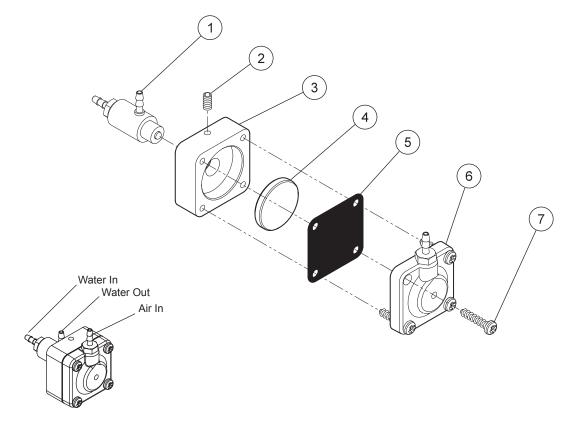

Water Relay Valve 123-000


| ITEM | PART DESCRIPTION PART NUMBER | QTY |
|------|--------------------------------|-----|
| 1 | Cartridge Body Assembly123-018 | 1 |
| 2 | Set Screw, 4-40 x 5/8"005-028 | 1 |
| 3 | Body123-013 | 1 |
| 4 | Piston123-014 | 1 |
| 5 | Diaphragm127-031 | 1 |
| 6 | Cap123-012 | 1 |
| 7 | Screw, #6 x 1/2"001-267 | 4 |
| 8 | Barb, 10-32 x 1/16"022-009 | 1 |
| 9 | Plastic Washer, 1/4"003-001 | 1 |
| 10 | Valve Body123-017 | 1 |
| 11 | Spring008-011 | 1 |
| 12 | O-Ring, 002017-502 | 1 |
| 13 | O-Ring, 001 017-501 | 2 |
| 14 | Stem 123-015 | 1 |

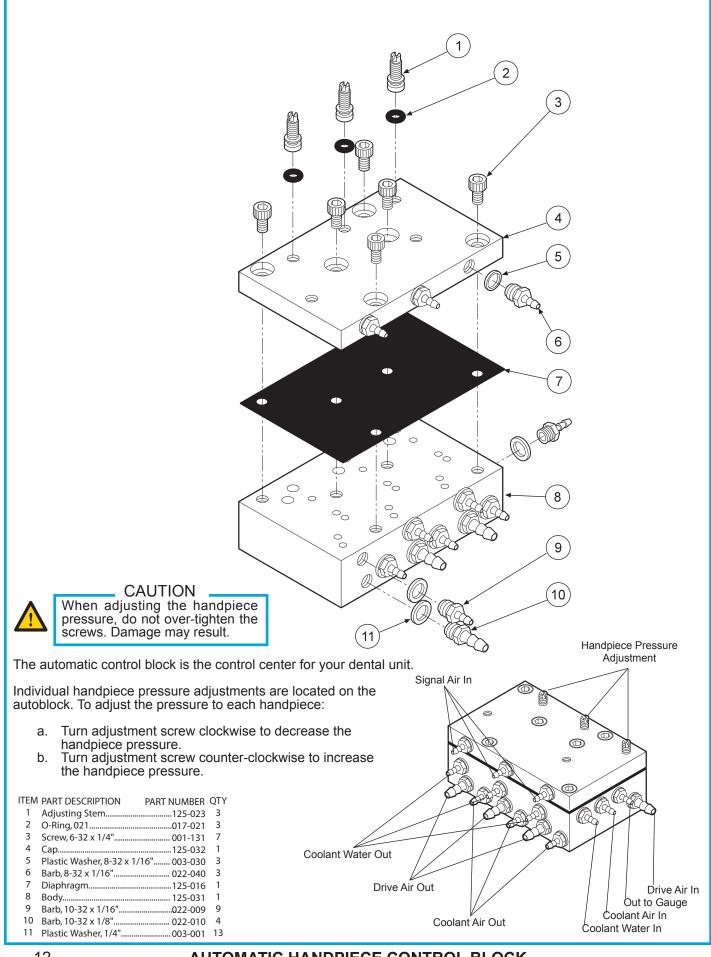

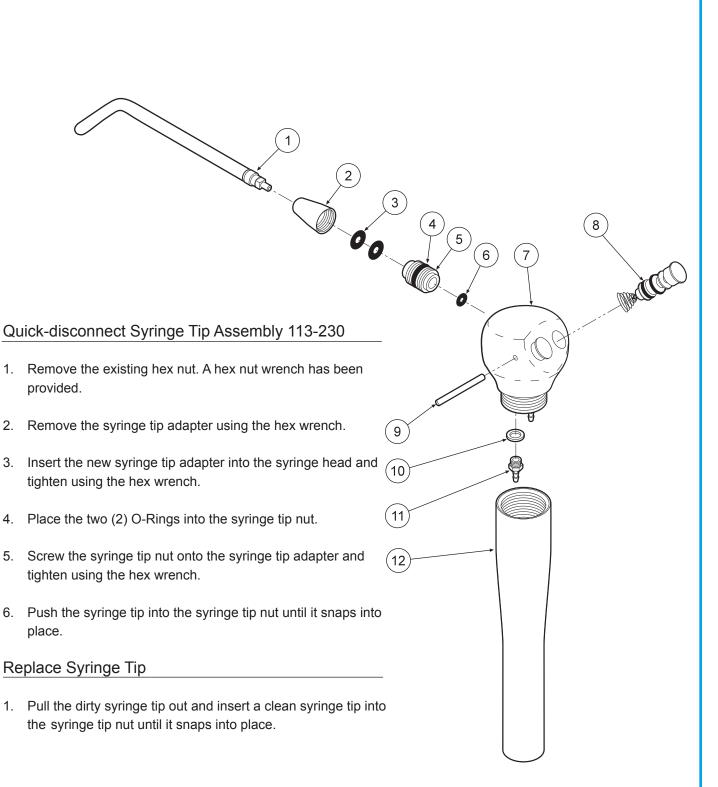

| 1TEM 1 2 3 4 5 6 7 8 9 10 | PART DESCRIPTION Syringe Tip | | QTY 1 1 2 1 1 1 1 2 1 2 1 2 |
|------------------------------|--------------------------------------|---------|-----------------------------|
| 9 | Pin, Syringe Cartridge | 113-008 | 1 |
| 10 11 12 | Barb, 8-32 x 1/16" Syringe Handle | 022-040 | 2 |


2.

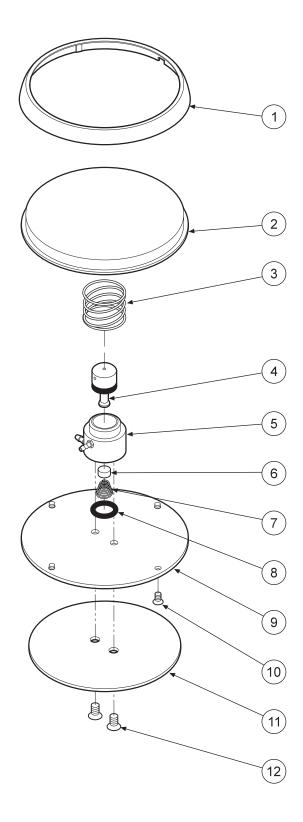

| ITEM | PART DESCRIPTION PART NUMBER | ≀ QTY |
|------|--|-------|
| 1 | Ring126-202 | 2 1 |
| 2 | Cover126-201 | 1 |
| 3 | Spring008-005 | 5 1 |
| 4 | Stem (Includes 017-012 o-ring)1.26-005 | 5 1 |
| 5 | Body126-004 | 1 1 |
| 6 | Poppet126-006 | 5 1 |
| 7 | Spring008-006 | 5 1 |
| 8 | O-Ring, 013017-013 | 3 1 |
| 9 | Baseplate126-003 | 3 1 |
| 10 | Screw, 4-40 x 1/4"001-005 | 5 4 |
| 11 | Rubber Pad 126-007 | 7 1 |
| 12 | Screw, 6-32 x 1/4"001-004 | 4 2 |
| | | |




3 Handpiece Automatic Slide Out Panel Mount

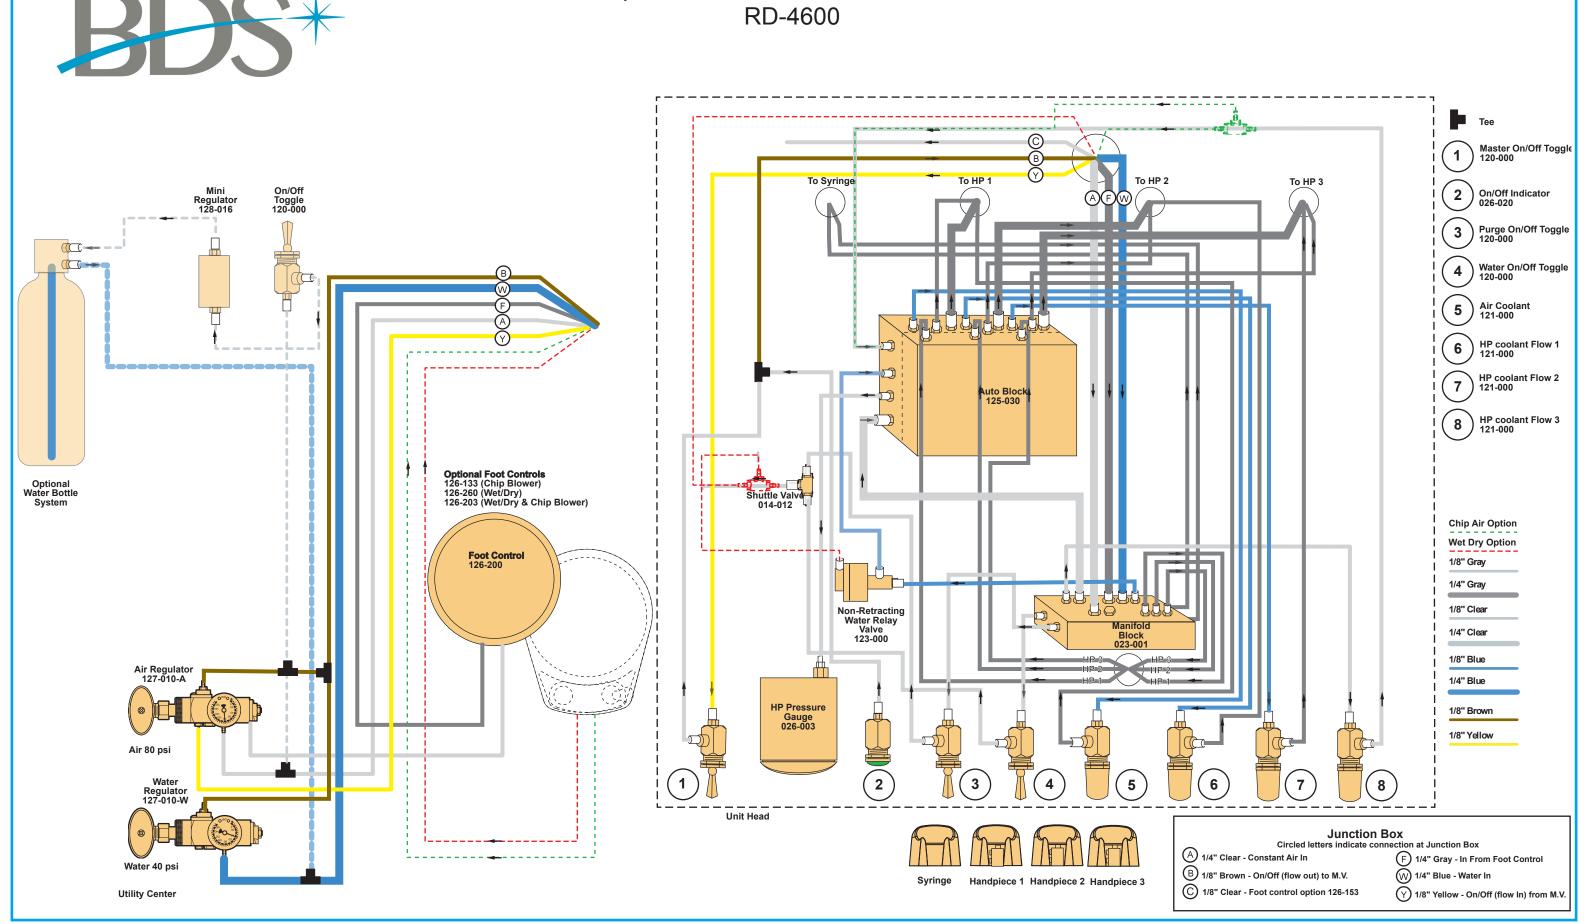



UNDER COUNTER MOUNT TEMPLATE

PM-4501, PM-4551, RD-4600, RD-4650

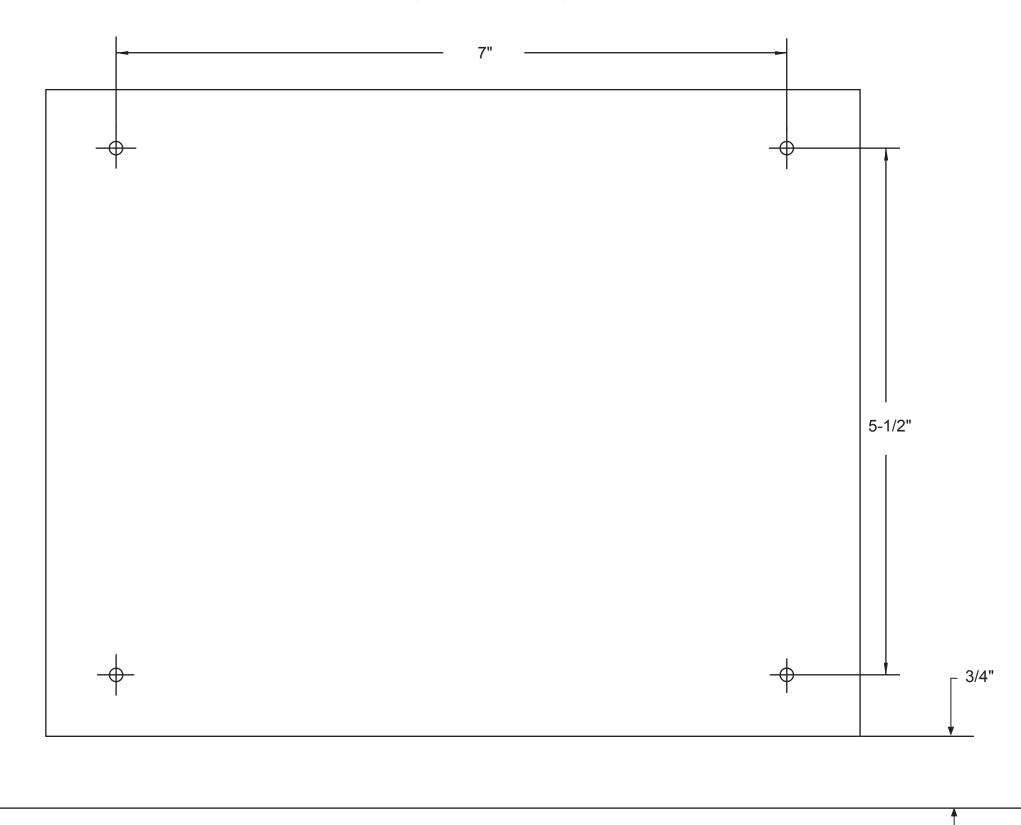


Rev 2 - 6-17-19

Front Edge —



CUTOUT TEMPLATE

for PM-4500, PM-4550, PM-4501, PM-4551

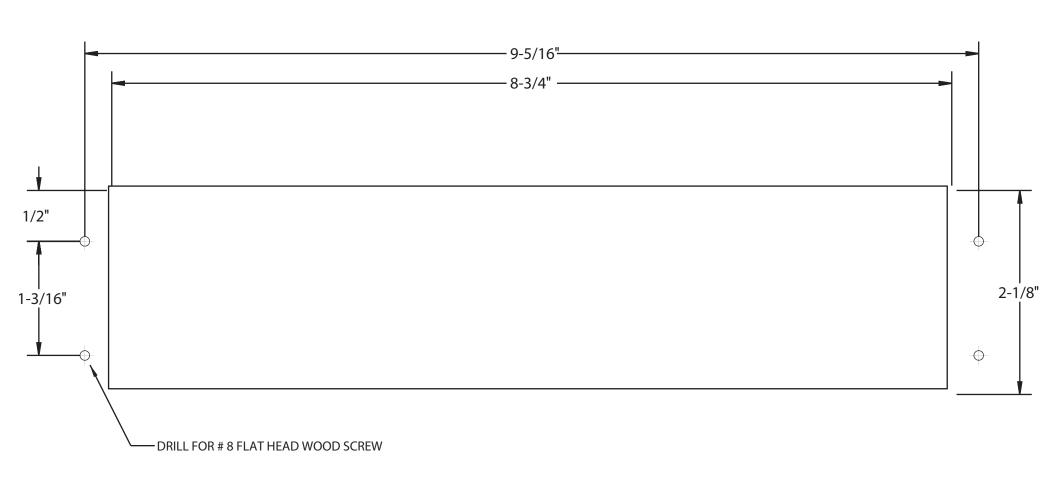

WARRANTY BDS warranties its product to be free of defects in material and workmanship for SEVEN FULL YEARS from the date of purchase on all units. Auto-blocks and standard foot controls are covered by a LIFETIME warranty when factory installed as part of a complete dental system. Upholstery has a TWO YEAR warrany and does not cover normal wear, stains, cuts or tears. Our LED lights have a FIVE year Warranty and our halogen light has a ONE year Warranty. Operatory chair motors feature a TEN year warranty. All warranty is limited to repair or replacement by BDS. Products returned to the factory and determined to be defective will be repaired or replaced free of charge at discretion of BDS. The warranty does not cover light bulbs, electrical components and trimmed or installed tubing. BDS reserves the right to void all warranties if any product is installed by other than an authorized technician. BDS' warranty does not cover damage to any surface finish, including but not limited to, discoloration or abrasion from cleaners, disinfectants or light sources. No claim for labor or consequential damages will be allowed. Return items must include a copy of the invoice or packing slip as proof of purchase.

Beaverstate Dental Inc. 115 S. Elliott Rd. Newberg, OR 97132 800-237-2303 503-538-8756 503-538-2845 Fax www.beaverstatedental.com